

# MODIFICATION RECOMMENDED

## L4451A-02

# S E R V I C E N O T E

Supersedes:  
NONE

## L4451A 4-Channel Isolated D/A Converter with Waveform Memory

Serial Numbers: MY00000000 through MY55210100

**Instrument cannot operate in 400 Hz**

### Parts Required:


P/N	Description	Qty.
L4421-84303	L44xxA Power Rating Label	1

## ADMINISTRATIVE INFORMATION

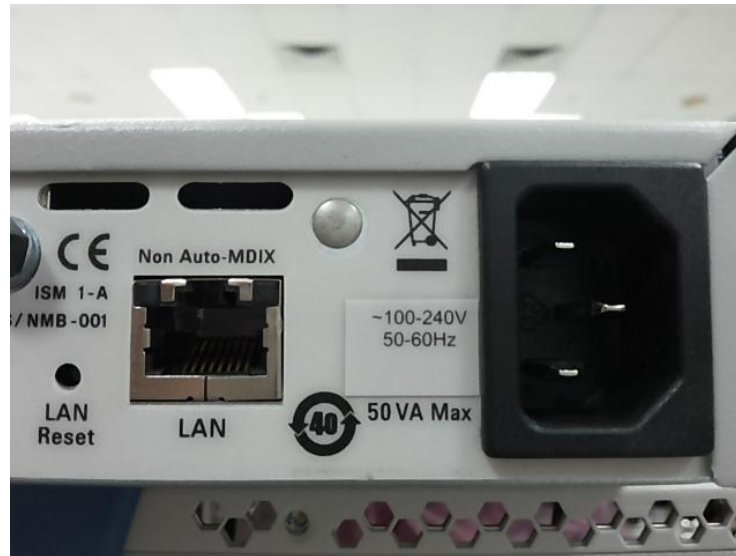
SERVICE NOTE CLASSIFICATION: <b>MODIFICATION RECOMMENDED</b>		
ACTION X ON SPECIFIED FAILURE CATEGORY: <input type="checkbox"/> AGREEABLE TIME	STANDARDS LABOR: 0.5 Hours	
LOCATION X CUSTOMER INSTALLABLE CATEGORY: <input type="checkbox"/> ON-SITE ( <b>active On-site contract required</b> ) X SERVICE CENTER <input type="checkbox"/> CHANNEL PARTNER	SERVICE X RETURN INVENTORY: <input type="checkbox"/> SCRAP <input type="checkbox"/> SEE TEXT	USED X RETURN PARTS: <input type="checkbox"/> SCRAP <input type="checkbox"/> SEE TEXT
AVAILABILITY: PRODUCT'S SUPPORT LIFE	NO CHARGE AVAILABLE UNTIL: End of Support	
<input type="checkbox"/> Calibration Required X Calibration NOT Required	PRODUCT LINE: BL AUTHOR: TP	
ADDITIONAL INFORMATION:		

**Situation:**

It has been found that the instruments with affected serial numbers listed above have incorrect information printed on the power rating label. The instrument does NOT support 400 Hz operation at 100-127V.

**Solution/Action:**

Order a L4421-84303 L44xxA Power Rating Label and apply it over the existing power rating information on the instrument. After applying the L4421-84303 label, it should look similar to the picture below.

**Revision History:**

Service Note Revision	Date	Author	Reason For Change
01	2015-07-02	TP	As published